

Selection of weighting factors for quantification of PET radioligand binding using simplified reference tissue models with noisy input functions

This article has been downloaded from IOPscience. Please scroll down to see the full text article.

2012 Phys. Med. Biol. 57 609

(<http://iopscience.iop.org/0031-9155/57/3/609>)

View [the table of contents for this issue](#), or go to the [journal homepage](#) for more

Download details:

IP Address: 128.36.136.143

The article was downloaded on 06/02/2012 at 17:34

Please note that [terms and conditions apply](#).

Selection of weighting factors for quantification of PET radioligand binding using simplified reference tissue models with noisy input functions

M D Normandin^{1,2,5}, R A Koeppe³ and E D Morris^{1,2,4,6}

¹ Weldon School of Biomedical Engineering, Purdue University, West Lafayette, IN, USA

² Department of Radiology, Indiana University School of Medicine, Indianapolis, IN, USA

³ Department of Radiology, University of Michigan, Ann Arbor, MI, USA

⁴ Department of Biomedical Engineering, Indiana University–Purdue University Indianapolis, Indianapolis, IN, USA

E-mail: normandin@pet.mgh.harvard.edu

Received 24 June 2011, in final form 21 October 2011

Published 12 January 2012

Online at stacks.iop.org/PMB/57/609

Abstract

Input function noise contributes to model-predicted values and should be accounted for during parameter estimation. This problem has been examined in the context of PET data analysis using a noisy image-derived arterial input function. Huesman and Mazoyer (1987 *Phys. Med. Biol.* **32** 1569–79) incorporated the effect of error in the measured input function into the objective function and observed a subsequent improvement in the accuracy of parameters estimated from a kinetic model of cardiac blood flow. Such a treatment has not been applied to the reference region models commonly used to analyze dynamic positron emission tomography data with receptor–ligand tracers. Here, we propose a strategy for selection of weighting factors that accounts for noise in the reference region input function and test the method on two common formulations of the simplified reference tissue model (SRTM). We present a simulation study which demonstrates that the proposed weighting approach improves the accuracy of estimated binding potential at high noise levels and when the reference tissue and target regions of interest are of comparable size. In the second simulation experiment, we show that using a small, homogeneous reference tissue with our weighting technique may have advantages over input functions derived from a larger (and thus less noisy), heterogeneous region with conventional weighting. A comparative analysis of clinical [¹¹C]flumazenil data found a small but significant increase in estimated binding potential when using the proposed weighting method, consistent with the finding of reduced negative bias in our simulation study. The weighting

⁵ Present address: Division of Nuclear Medicine and Molecular Imaging, Department of Radiology, Massachusetts General Hospital and Harvard Medical School, Boston, MA 02114, USA.

⁶ Present address: Department of Diagnostic Radiology, Yale University School of Medicine, New Haven, CT 06515, USA.

strategy described here accounts for noise in the reference region input function and may improve the performance of the SRTM in applications where data are noisy and the reference region is relatively small. This technique may offer similar benefits to other models using reference region inputs, particularly those derived from the SRTM.

(Some figures in this article are in colour only in the electronic version)

1. Introduction

Positron emission tomography (PET) imaging with receptor–ligand tracers has been used extensively to study neuroreceptor density and distribution *in vivo*. Quantification is typically achieved by the calculation of binding potential (BP_{ND}), which reflects the equilibrium ratio of specific binding to non-displaceable tracer uptake and serves as an index of receptor availability (see Innis *et al* 2007 for review). BP_{ND} was first introduced to the imaging community as an outcome of the two-tissue compartment model (Mintun *et al* 1984) (see figure 1(a)). This model reflects the transfer of tracer molecules between distinct states (i.e. suspended in plasma, free in tissue, or bound to receptors) over time. Using a measured arterial input function, one can determine the rate constants describing these transitions. BP_{ND} can then be calculated from the estimated model parameters.

The full reference region model (Blomqvist *et al* 1990, Cunningham *et al* 1991) (see figure 1(b)) derives the input function to the two-tissue compartment model from image data measured in a reference region devoid of receptors. The full reference tissue model eliminates the need for arterial blood sampling, significantly reducing the cost, complexity and invasiveness of experiments. However, the computational burden of the requisite nonlinear data fitting prohibits voxel-by-voxel analysis, and parameter identifiability is often unsatisfying (Lammertsma and Hume 1996, Gunn *et al* 1997).

The simplified reference tissue model (SRTM) (Lammertsma and Hume 1996) reduces the number of estimated parameters by collapsing the two tissue compartments of the target region into a single apparent compartment as depicted in figure 1(c). The reduction in the number of unknown variables improves parameter identifiability. Computation time is also decreased, but remains formidable because nonlinear parameter estimation is still required. Two common implementations of the SRTM that greatly improve its computational efficiency are the basis function method (BFM) (Gunn *et al* 1997) and the multilinear reference tissue model (MRTM) (Ichise *et al* 2003) (also derived independently by Alpert *et al* (2003) and Zhou *et al* (2003)).

The BFM and MRTM parameters are typically obtained by weighted least-squares estimation, with each residual (i.e. the difference between measured and model-predicted values) weighted according to an approximation of the variance of the corresponding target region PET datum. Weighted least-squares is recommended when measurements are not uniformly reliable, as is the case for dynamic PET data. Each squared residual term in the objective function should be normalized by a factor proportional to its variance in order to construct an unbiased estimator. Selecting these weights based solely on the variance of the target region data implicitly assumes that the model predictions do not contribute to the uncertainty of the residuals. The measured input function must be noiseless to satisfy this condition. Fitting the input data to a smooth curve prior to analysis is insufficient because

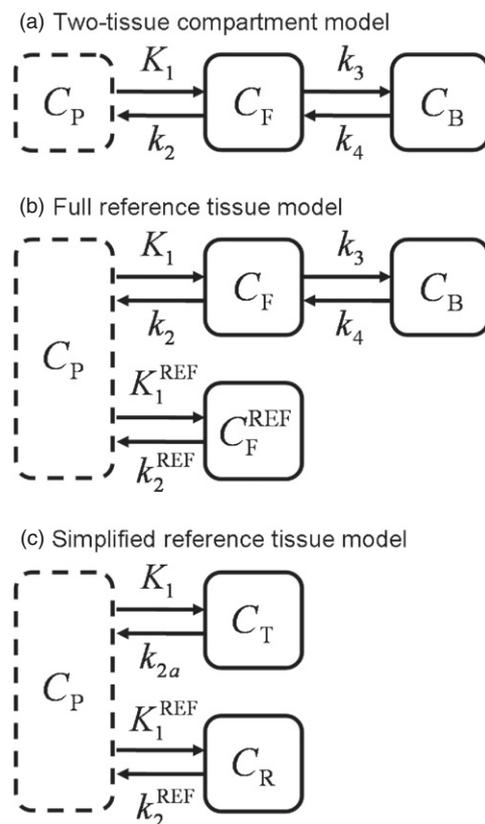


Figure 1. Compartmental models commonly applied to dynamic receptor–ligand PET data. (a) The two-tissue compartment model uses a plasma input function and expresses tracer kinetics in terms of transitions between plasma (C_P), free (C_F) and bound (C_B) states. (b) The full reference tissue model uses the two-tissue model to describe the target region and derives the input function from data acquired in a reference region (C_F^{REF}). (c) The simplified reference tissue model uses a reference region input and collapses the two tissue compartments of the target region into a single apparent compartment (C_T).

statistical uncertainties propagate from the estimated input function parameters to the model-predicted target region values (Huesman and Mazoyer 1987). If the assumption of an exact input function is not valid, then the weighting factors for each residual are incorrect. Improper selection of weights introduces error into the objective function (Spilker and Vicini 2001).

Huesman and Mazoyer examined the problem of noisy image-derived arterial input functions on the analysis of ^{82}Rb cardiac PET data with a blood flow model (Huesman and Mazoyer 1987). They incorporated the uncertainty attributable to input function noise into the covariance matrix used to weight the residuals during parameter estimation, a method later proven (Huesman 1997) to be mathematically equivalent to extending the objective function with parameters describing the noisy input data (Chen *et al* 1991, Chiao *et al* 1994). Their approach produced a reduction in the bias of estimated parameters and a moderate improvement in their precision. Previous studies have evaluated the choice of weights for the SRTM (Muzic and Christian 2006, Thiele and Buchert 2008, Tomasi *et al* 2008a) but did not address the effect of noise in the reference region data. To our knowledge, the reference region PET

models have not been scrutinized with respect to the proper assignment of weighting factors given a noisy input function, although the potential need to do so has been recognized in the literature (Aston *et al* 2000, Ichise *et al* 2003, Zhou *et al* 2003).

The purpose of this work is to adapt the method of Huesman and Mazoyer to the BFM and MRTM implementations of the SRTM and to test its effect on quantification of binding potential. The BFM and MRTM models have received widespread application and the SRTM has inspired numerous extensions (Wu and Carson 2002, Alpert *et al* 2003, Ichise *et al* 2003, Zhou *et al* 2003, 2006, Ichise *et al* 2008, Tomasi *et al* 2008b, Møller *et al* 2009, Ikoma *et al* 2009, Normandin *et al* 2011) to which this weighting strategy might also be applicable.

2. Theory

2.1. Simplified reference tissue model

The kinetics of receptor–ligand tracers are often described in terms of the two-tissue compartment model (see figure 1(a)), which describes the transitions of tracer between distinct states: suspended in the plasma, free in the tissue, or bound to receptors. The mass balance equations that comprise the model are

$$\frac{dC_F(t)}{dt} = K_1 C_P(t) - (k_2 + k_3) C_F(t) + k_4 C_B(t) \quad (1)$$

and

$$\frac{dC_B(t)}{dt} = k_3 C_F(t) - k_4 C_B(t), \quad (2)$$

where the state variables reflect concentration of the tracer in the respective compartments.

If PET data are measured in a reference tissue devoid of receptors, the relevant mass balance on free tracer is

$$\frac{dC_F^{\text{REF}}(t)}{dt} = K_1^{\text{REF}} C_P(t) - k_2^{\text{REF}} C_F^{\text{REF}}(t). \quad (3)$$

If such a reference region exists, equation (3) can be rearranged to yield an approximation for the plasma input function, $C_P(t)$, in terms of the PET data measured in the reference region. The two-tissue compartment model with a reference region input constitutes the full reference tissue model (figure 1(b)). The SRTM (figure 1(c)) uses a reference region input function and collapses the two tissue compartments of the target region into a single apparent compartment. The mass balance on tracer in the target region is then

$$\frac{dC_T(t)}{dt} = K_1 C_P(t) - k_{2a} C_T(t), \quad (4)$$

where k_{2a} (min^{-1}) is the apparent efflux rate from the collapsed tissue compartment. The model output can be expressed as

$$C_T(t) = R_1 C_R(t) + \left(k_2 - \frac{R_1 k_2}{1 + B P_{\text{ND}}} \right) C_R(t) * \exp \left(\frac{-k_2 t}{1 + B P_{\text{ND}}} \right), \quad (5)$$

where $R_1 = K_1 / K_1^{\text{REF}}$ (unitless), k_2 (min^{-1}) is interpreted in the two-tissue model sense (i.e. $k_2 = R_1 k_2^{\text{REF}}$) and $*$ denotes the convolution operator.

The BFM and MRTM are two common variants for fitting the SRTM to data. The BFM groups the model into linear and nonlinear components and defines basis functions that replace the nonlinear term. Thus the model is restated as

$$C_T(t) = \theta_1 C_R(t) + \theta_2 C_R(t) * \exp(-\theta_3 t). \quad (6)$$

By discretizing θ_3 over a range of plausible values, basis functions of the form $B_i(t) = C_R(t) * \exp(-\theta_3 t)$ can be created. Equation (6) then simplifies to

$$C_T(t) = \theta_1 C_R(t) + \theta_2 B_i(t) \tag{7}$$

from which θ_1 and θ_2 can be readily determined using linear algorithms. The basis function that yields the best model fit to the data corresponds to a unique set of parameters $(\theta_1, \theta_2, \theta_3)$ from which the optimal model parameters (R_1, k_2, BP_{ND}) are obtained by substitution. By contrast, the MRTM is an integral formulation of the SRTM in which all parameters are linear coefficients. Its operational equation is

$$C_T(t) = R_1 C_R(t) + k_2 \int_0^t C_R(u) du - k_{2a} \int_0^t C_T(u) du \tag{8}$$

with the variables defined as above. Binding potential can be calculated from the relationship $BP_{ND} = k_2/k_{2a} - 1$.

The parameters of equations (7) and (8) are typically obtained by minimizing the weighted sum of squared residuals, $\sum_{i=1}^n w_i (d_i - m_i)^2$. The residuals represent the differences between the measured data, d_i , and the model predicted values, m_i . According to estimation theory, the weighting factors, w_i , should be set inversely proportional to the variance of each residual. In practice, the weighting factors are usually chosen according to an approximation of the variance of the PET data measured in the target region. This approach treats the uncertainty of the residuals as entirely attributable to the statistical noise of the target region data. Thus, the model output is assumed to be certain and generated by a noiseless input function. In the following section, we propose an alternative weighting strategy which, in addition to error in the target region, also accounts for the contribution of uncertainty in the reference region measurements to the total variance of the residuals in the objective function.

2.2. Selection of weighting factors

Assuming Poisson noise properties (Snyder 1973, Landaw and DiStefano 1984, Mazoyer *et al* 1986) and a sufficiently large number of events, the variance of the tracer concentration in a region of interest (ROI) can be approximated by

$$\sigma_{i,ROI}^2 = \zeta^2 \frac{C_{ROI}(t_i)}{n_{ROI} \Delta t_i}, \tag{9}$$

where C_{ROI} is the measured concentration in the ROI, Δt is the length of the time frame, n_{ROI} is the number of voxels in the ROI, ζ^2 is a scale factor, and i indexes the PET time frames. If we assume that (i) the convolution term of equation (6) and the integral terms of equation (8) are effectively noiseless (Ichise *et al* 2002, Zhou *et al* 2003), (ii) the noise in the reference and target regions is uncorrelated, and (iii) if ζ is the same in the target and reference regions, then the variance of the residuals can be approximated by

$$\sigma_{i,resid}^2 = \frac{\zeta^2}{\Delta t_i} \left[\frac{C_T(t_i)}{n_T} + R_1^2 \frac{C_R(t_i)}{n_R} \right], \tag{10}$$

where the subscripts T and R refer to the target and reference regions, respectively. A derivation is provided in appendix A. In this paper, we use the term Standard weighting to designate selection of weights according to the variance approximated by equation (9), where ROI refers to the target region only, and define Reference weighting to be the selection of weights according to the expression for variance in equation (10), which includes contributions from both the target and reference regions.

3. Methods

3.1. Simulation studies

Computer simulations and analyses were performed in GNU Octave (Eaton 2002). Reference and target region data were simulated using a one-tissue compartment model with kinetics similar to moderate affinity receptor–ligand tracers such as [¹¹C]raclopride and [¹¹C]flumazenil. True binding potential in the target region was set equal to 2.0. Poisson-like noise (see equation (9)) was added to the noiseless data to generate 500 pairs of target and reference region curves at each of 11 noise levels (1.6% to 16% fractional standard deviation at a peak of the target region curve) and 11 reference-to-target region volume ratios ($\frac{1}{3} \leq n_R/n_T \leq 100$). Example time activity curves at different noise levels are shown in appendix B.

3.1.1. Comparison of weighting methods. The BFM and MRTM models were fit to the simulated data using a weighted least-squares approach with either Standard or Reference weighting. As can be seen from equation (10), the Reference weighting factors depend on the value of the model parameter R_1 . The Reference weights were therefore determined in two different ways. In one, the weights were determined with R_1 fixed at 1 (true value = 1.2). The model was then applied in the usual fashion with R_1 as an estimated parameter. In the other, the model was applied iteratively with the Reference weights updated based on the value of R_1 estimated at the most recent iteration. The initial guess for R_1 was 1 and convergence was determined using a relative tolerance of 10^{-3} . As done previously (Ichise *et al* 2003, Wu and Carson 2002), fits were considered outliers if the estimated value of either R_1 or BP_{ND} was negative or greater than five times the true value. The comparisons performed in this study tested the hypothesis that the SRTM would perform better using Reference weighting factors than with Standard weights.

3.1.2. Comparison of reference regions. We considered that a hypothetical region comprised of two kinetically distinct and separable tissue types: one that was an ideal reference tissue with no specific binding, and a non-ideal one having kinetics consistent with a receptor density equal to 10% of the target region. The reference region used to obtain the input function was either the ideal reference tissue alone or the sum of the ideal and non-ideal tissues. Thus, the first curve had ideal reference tissue kinetics, but was obtained from a smaller region and was therefore unbiased but noisy, whereas the second curve was biased but with better signal to noise. The BFM and MRTM models were fit to the data as described above, using Standard weighting with the input derived from the larger region or Reference weighting with the input function derived from the smaller region. The purpose of this comparison was to determine whether Reference weighting would justify the selection of smaller, more homogeneous reference regions.

3.2. Positron emission tomography studies

PET data were acquired dynamically from 25 healthy human subjects after injection of [¹¹C]flumazenil, a central benzodiazepine receptor ligand. One group of 17 subjects underwent single PET scans on an ECAT Exact HR+ scanner (Siemens Medical Systems, Knoxville, TN). One group of four subjects underwent two PET scans each on an ECAT Exact 47 camera (Siemens Medical Systems, Knoxville, TN). Another group of four subjects underwent two PET scans each, once during a baseline condition and with a blocking dose of unlabeled flumazenil. Two of these subjects were scanned on the HR+ and two were scanned with

the Exact-47. All data were acquired in 3D mode and binned into 15 sinograms with the following time frames: 4×30 s, 3×60 s, 2×150 s, 2×300 s, 4×600 s. Images were reconstructed with corrections for scatter, attenuation, dead time and detector non-uniformity using an ordered subset expectation maximization (OSEM) algorithm (4 iterations, 16 subsets) for data acquired on the HR+ or filtered backprojection (Hanning filter with 0.5 cutoff) for data acquired with the Exact-47. These studies were approved by the University of Michigan Institutional Review Board and all subjects provided informed consent.

Dynamic PET images were motion corrected and aligned to a stereotactic orientation using the NeuroStat image analysis software suite (Minoshima *et al* 1993, 1994). Time activity curves were extracted from each of 66 ROIs using a template based on the Talairach atlas. The BFM and MRTM models were applied to ROI data with Standard or Reference weights (calculated with $R_1 = 1$) using the pons as a reference region. The *in vivo* kinetics of [^{11}C]flumazenil are well described by a one-tissue compartment model (Koeppel *et al* 1991), so use of the SRTM is entirely justified.

Fractional differences between BP_{ND} values estimated with Standard or Reference weights were compared using the Wilcoxon matched-pairs signed-ranks test. The within-region variance of BP_{ND} estimated using either weighting scheme was determined across subjects in the baseline condition. We note that values of BP_{ND} are expected to vary not only between regions, but also between subjects for a given region. Hence the within-region measure of variance reflects intersubject variability as well as the intrinsic uncertainty of BP_{ND} estimates. On the other hand, the implicit parameter $k_2^{\text{REF}} (= k_2/R_1)$ should theoretically be constant across regions within a given data set because there is only one reference region curve for each scan (Wu and Carson 2002, Ichise *et al* 2003). For this reason, the within-scan variability of k_2^{REF} across regions was calculated as an alternative indicator of the precision of model parameters.

4. Results

4.1. Simulation study: comparison of weighting methods

4.1.1. Reference weighting with R_1 fixed. Figure 2 shows the bias ((a) and (b)) and precision ((c) and (d)) of BP_{ND} estimated by BFM with either Standard weighting or Reference weights calculated with R_1 fixed. In each subplot, the noise level increases moving toward the right and the size of the target region relative to the reference regions decreases moving toward the top. BP_{ND} was negatively biased and more variable at high noise levels for both weighting approaches. Reference weighting improved the accuracy (figure 2(e)) and to a lesser extent the precision (figure 2(f)) of estimated BP_{ND} as compared to Standard weighting, as shown in the difference maps of figures 2(e) and (f), where positive values indicate lower bias and variance for results of the Reference weighting method. The advantage became more pronounced as noise increased and the relative size of the reference region decreased, reaching maximum effect at the highest noise level and when the reference tissue was smaller than the target region (lower right of each plot). There was little impact on performance with large reference regions or at low noise levels. Similarly, MRTM was more accurate (figure 3(e)) with Reference than Standard weighting, although improvement in absolute precision was less pronounced (figure 3(f)).

4.1.2. Reference weighting with R_1 updated iteratively. Similar to Reference weighting using a value for fixed R_1 , the bias and variability of BP_{ND} were smaller using Reference

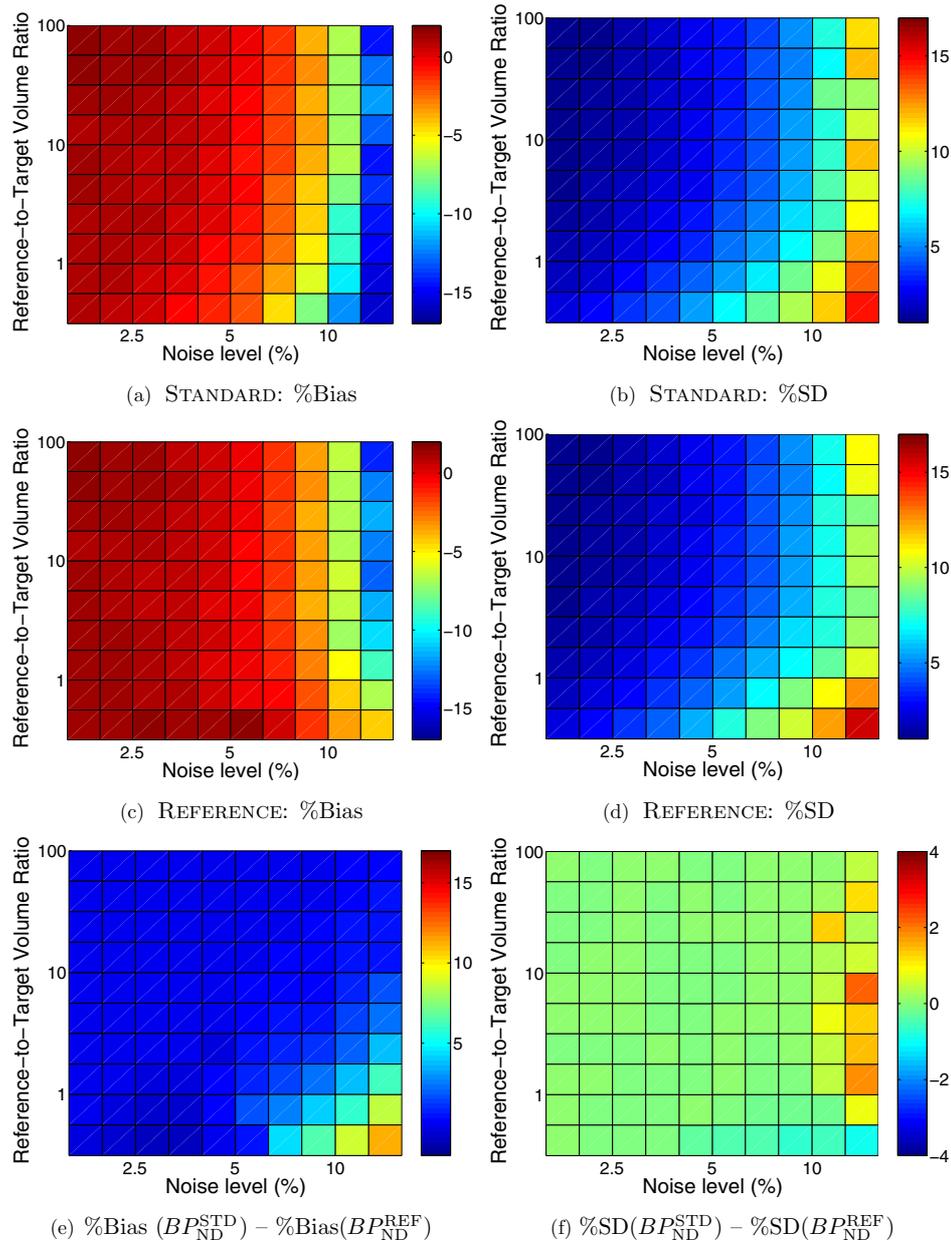


Figure 2. Comparison of bias and standard deviation of BP_{ND} values estimated by BFM using Standard weighting or Reference with R_1 fixed. In each subplot, noise increases moving toward the right and the size of the target region relative to the reference region decreases moving toward the top. Bias and standard deviation are indicated by the color scale and expressed as percentages relative to the true value of BP_{ND} . (a), (c) and (e) each cover a range of 20 percentage points to facilitate comparisons. (b) and (d) are scaled alike, but (f) spans a smaller range (8 versus 20 percentage points) to aid visualization. In the difference plots of (e) and (f), greater values indicate better performance by Reference than Standard weighting. Improvements in bias and precision were most pronounced at high noise levels and when the target and reference regions were of similar size. Figure C1 presents a subset of these results for selected region sizes as plots of bias \pm s.d. as a function of noise level.

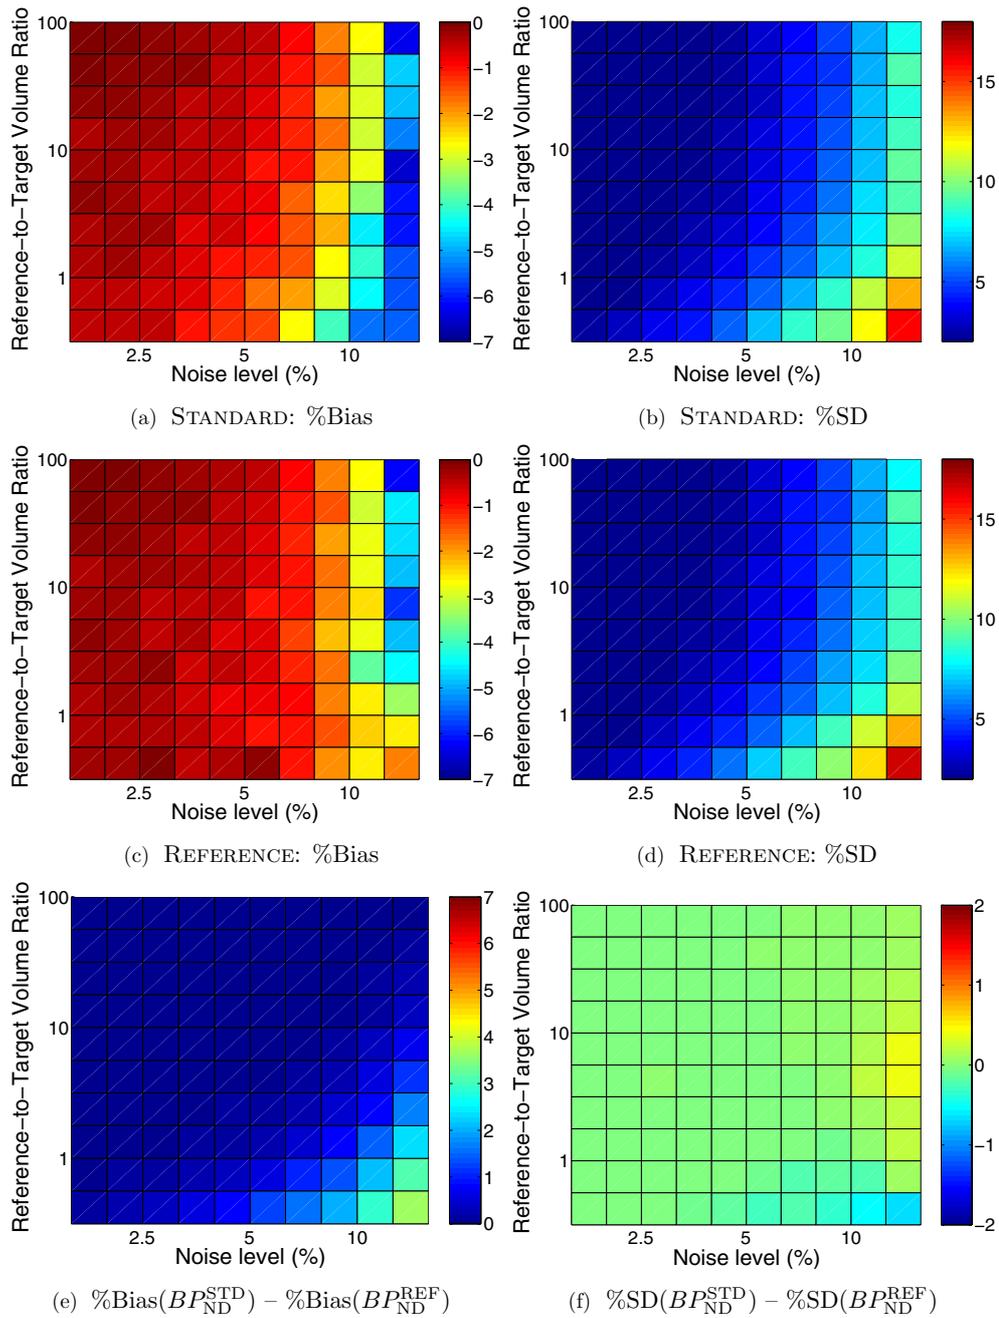


Figure 3. Comparison of BP_{ND} estimated with Standard or Reference (R_1 fixed) weighting using MRTM, presented as in figure 1. (a), (c) and (e) share a common scale. (b) and (d) are scaled alike, but (f) spans a smaller range to aid visualization. Bias and standard deviation are expressed as percentages relative to the true value of BP_{ND} . Figure C2 presents a subset of these results for selected region sizes as plots of bias \pm s.d. as a function of noise level.

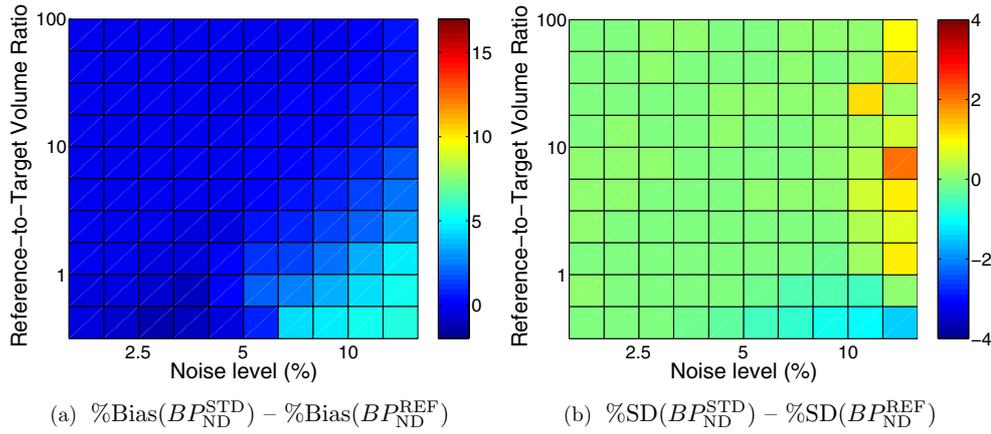


Figure 4. Comparison of accuracy and precision in BP_{ND} estimated by BFM using Standard weighting or Reference weighting with R_1 updated iteratively. Difference plots for (a) bias and (b) standard deviation are presented as in figures 2 (e) and (f), where greater values indicate lower bias and better precision with the Reference weighting method. Comparing (a) and (b) directly to figures 2 (e) and (f) (note the matching scales) indicates that the performance of Reference with R_1 iterated was intermediate between Standard and Reference with R_1 fixed. Results with MRTM were similar.

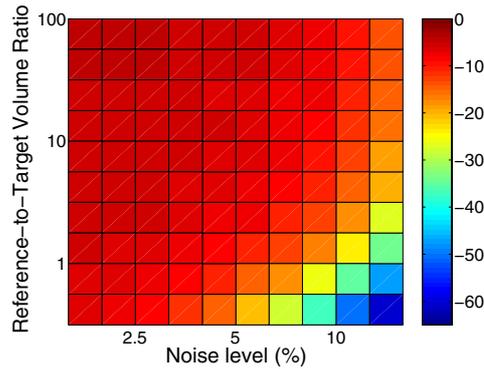


Figure 5. Bias in R_1 using Reference with R_1 updated iteratively. Underestimation of R_1 de-emphasizes the contribution of the reference region to the calculated variance of residuals (see equation (10)). Thus, the performance of Reference with R_1 iterated was intermediate between Standard weighting and Reference with R_1 fixed (figures 2(e) and (f), 4(a) and (b)).

weighting with R_1 iterated than using Standard weighting. The greatest reductions in bias and variability occurred when noise was high and the target and reference regions were of similar size (figure 4), where greater values indicate improved performance with Reference weighting. Comparing these results to those shown in analogous difference plots of figures 2(e) and (f) indicates that Reference weighting improved accuracy more when factors were calculated with R_1 fixed than with R_1 iterated (note that the scales of figures 2(e) and 4(e) are identical). The precision was similar for either variant of Reference weighting. Trends were comparable for MRTM (not shown). R_1 was increasingly underestimated as noise increased and as the volume of the reference region decreased (figure 5).

4.2. Simulation study: comparison of reference regions

Even at low noise levels, negative bias in BP_{ND} estimated with BFM was considerable ($\sim 14\%$, see figure 6(a)) when data from the large, heterogeneous reference region were used as the input function with Standard weighting. In contrast, the smaller (but kinetically ideal) tissue with Reference weighting yielded essentially unbiased estimates of BP_{ND} at low noise (figure 6(a)). BP_{ND} values obtained using Reference with the smaller region were less biased than those estimated using Standard with the larger region for all combinations of the noise level and region size (figure 6(e)). As expected, absolute precision was better for Standard with a large reference region, consistent with the higher signal-to-noise ratio of the input data. However, in terms of the coefficient of variation of BP_{ND} , the precision obtained using the small region with Reference weighting is comparable to that of the large region with Standard weighting, whereas the accuracy is better across all combinations of noise levels and region sizes.

4.3. Human imaging studies

BP_{ND} estimates obtained using Reference weighting were greater than values estimated using Standard weights for 1651 of 2177 curves (75.8%) via BFM and 1786 of 2176 (82.1%) data sets via MRTM. Of the 2178 analyzed target region curves (33 scans \times 66 regions per scan), one data set yielded negative BP_{ND} values with MRTM using both Standard and Reference weighting and was excluded from statistical analysis. One additional data set yielded unphysiological BP_{ND} values when analyzed by MRTM and was also excluded. The average increase in BP_{ND} with Reference weighting was small ($0.38\% \pm 0.53\%$ for BFM, $0.23\% \pm 0.31\%$ for MRTM) but highly significant ($p < 10^{-10}$, Wilcoxon matched-pairs signed-ranks test). Increases in BP_{ND} attributable to Reference weighting were greater for data sets acquired on the HR+ and reconstructed with OSEM ($0.41\% \pm 0.15\%$ for BFM, $0.25\% \pm 0.10\%$ for MRTM) than those acquired on the Exact-47 with FBP reconstruction ($0.33\% \pm 0.17\%$ for BFM, $0.22\% \pm 0.09\%$ for MRTM). No differences in the precision of BP_{ND} were observed between weighting approaches. Estimates of k_2^{REF} from either weighting method showed no substantial difference in absolute values (with BFM, mean across subjects, 0.31 ± 0.07 versus $0.30 \pm 0.07 \text{ min}^{-1}$; with MRTM, mean 0.28 ± 0.05 versus $0.27 \pm 0.05 \text{ min}^{-1}$) or variability (for BFM, mean within-subject fractional standard deviation equal 16.2 ± 6.5 versus $16.6\% \pm 6.9\%$ for MRTM, 15.5 ± 5.5 versus $16.2\% \pm 0.05\%$). For both BFM and MRTM, an inverse relationship was observed for the fractional difference in BP_{ND} between Reference and Standard weighting (i.e. the magnitude of Reference weighting's effect) and the volume of the reference region relative to the target region (figure 7), consistent with the findings of the simulation studies.

5. Discussion

We have demonstrated that accounting for noise in the input function when choosing weighting factors can improve the quantitation of binding potential with two common formulations of the SRTM. Our first simulation study indicated that the greatest improvement in performance occurred at high noise levels and when the target and reference regions were of similar size (figures 2 and 4). Analysis of region-of-interest data from [^{11}C]flumazenil experiments in humans using the pons as the reference tissue showed a small but highly significant increase in BP_{ND} using Reference as compared to Standard weighting. These results support the findings of our simulation study and demonstrate the statistical impact of Reference weighting

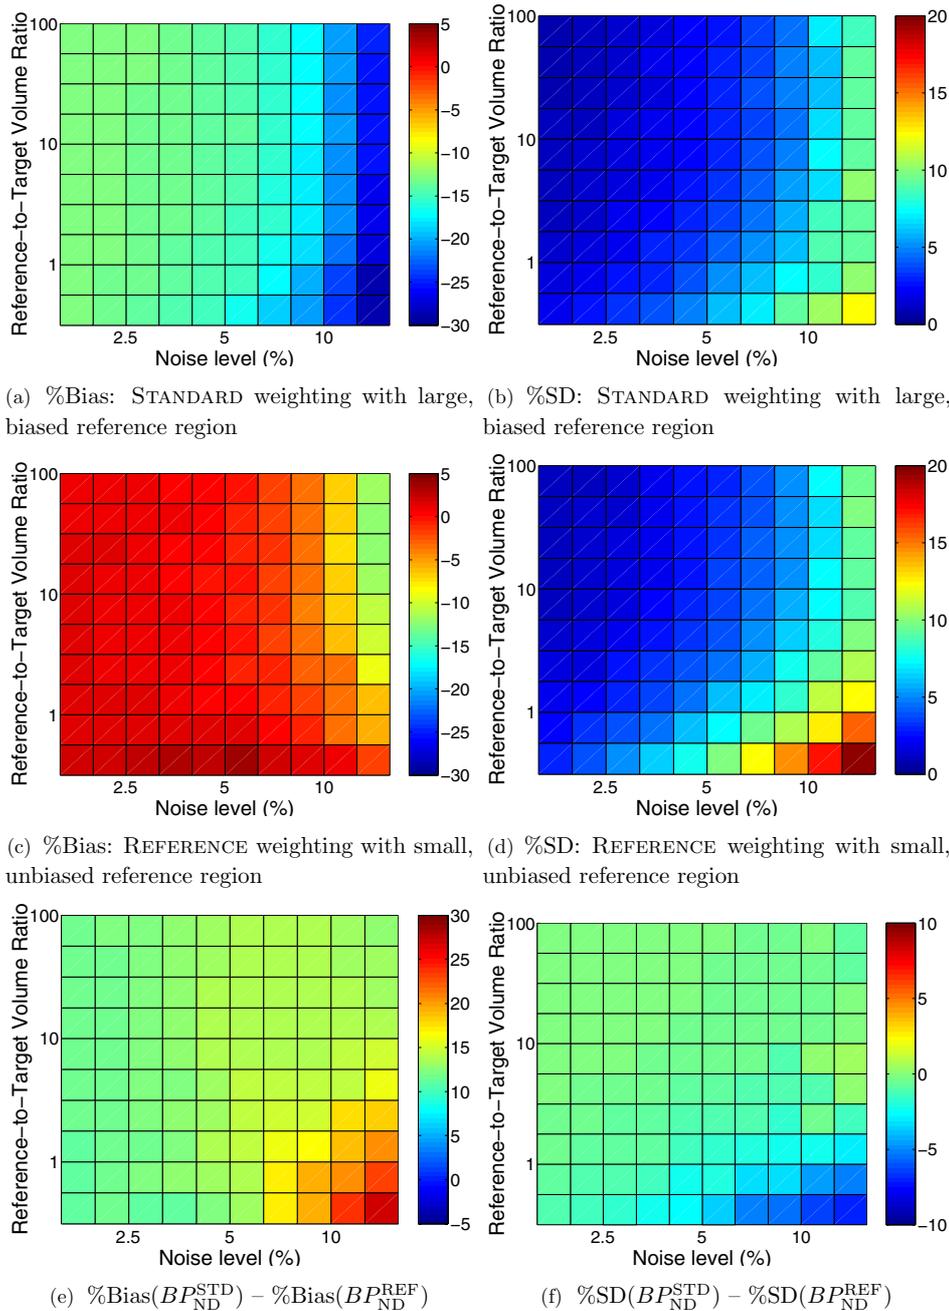


Figure 6. Comparison of accuracy and precision of BP_{ND} estimated by BFM using Standard weighting with a large, heterogeneous reference tissue biased by the presence of specific binding or Reference weighting (R_1 fixed) with small, ideal reference region. BP_{ND} values obtained with Standard weighting and biased input data were underestimated by 14% or more across all noise levels and region sizes, whereas values estimated with Reference weighting were essentially unbiased except at very high noise levels. Absolute variance was greater with Reference weighting, but the coefficient of variation was comparable to standard. Bias and standard deviation are expressed as percentages relative to the true value of BP_{ND} .

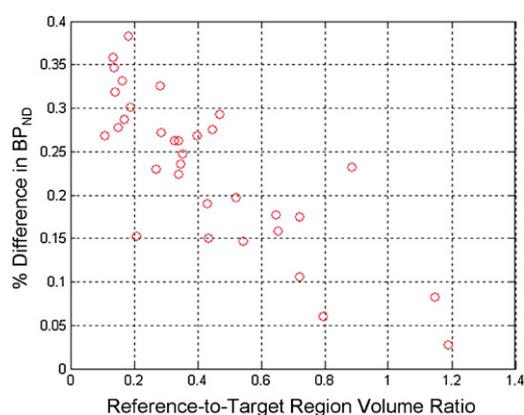


Figure 7. Percent increase in BP_{ND} estimated from human [^{11}C]flumazenil data using Reference compared to Standard weighting as a function of relative region size. Fractional change was averaged across all 33 scans for each of the 33 uniquely sized brain regions. The trend toward greater effect of Reference weighting for larger target region volumes is consistent with findings of the simulation studies. The linear regression fit was $y = -0.25x + 0.34$ and, though not strictly valid over a wider range of region sizes, adequately described the relationship with a correlation coefficient of $r = 0.69$.

on clinical data. However, the magnitude of the observed increase in BP_{ND} suggests that Reference weighting alone has a marginal effect at noise levels typically encountered in ROI-based analyses of human PET data. Thus, we posit that Reference weighting may be most beneficial for small animal imaging, when the noise level varies between data sets (due to differences in injected radioactivity, for example), or any time the statistical properties of the input function are especially poor. Similarly, this technique may be particularly useful when the amount of radioactivity must be limited for pharmacological reasons (e.g. with agonist tracers, high affinity ligands, or radiosyntheses yielding low specific activity) or to minimize radiation exposure.

A trend toward the greater effect of Reference weighting with larger target regions was observed in the [^{11}C]flumazenil data (figure 7), also consistent with simulation results. We note that the size of the reference tissue was fixed, whereas target regions of different volumes were analyzed. In contrast to simulation studies where we were able to manipulate region volume and noise level independently, for these experimental data the size of the target region influenced not only the relative volumes of the reference and target regions (the vertical position of the operating point in figures 2–6, with smaller target regions appearing nearer the top) but also the noise level of the target region data (the horizontal position, with noisier curves toward the right). In particular, according to the Poisson-like noise model, we expect that an n -fold change in the target region volume will yield a \sqrt{n} -fold reduction in the noise level. Given the topologies observed in figures 2–6, we cannot exclude the possibility that the [^{11}C]flumazenil curves generated from target regions of different sizes fell approximately along an isocontour, diminishing the relationship between the impact of the weighting method and relative region size.

The second of our simulation experiments indicated that analyses carried out with a smaller, unbiased reference tissue coupled with Reference weighting were more accurate than those using a larger, non-ideal reference region with Standard weighting, as is often done in practice to reduce noise in the input function. In terms of absolute precision (e.g.,

relative to the true parameter value), the estimates of BP_{ND} obtained with the larger reference region were less variable, consistent with the lower noise of that input curve. However, if variability is considered relative to the estimated parameter values (i.e. the coefficient of variation), the two approaches have similar precision. Therefore, both methods should have similar ability to differentiate populations, while the use of a smaller reference region with Reference weighting would offer the advantage of reduced bias for quantitative applications which benefit from accurate estimates of BP_{ND} and unbiased reference region data. The use of a smaller, more appropriate reference region could be envisioned when putative reference tissues are heterogeneous with subregions having specific binding or non-specific binding inconsistent with target tissues, or when the conventional reference region is susceptible to signal contamination from adjacent tissues (i.e. spillover due to partial volume effects).

5.1. Iteration of R_1

The model parameter R_1 appears in the Reference approximation of uncertainty in the residuals (equation (10)). We therefore considered two alternative approaches, either assigning the weights with R_1 fixed at an assumed (and in these simulations, incorrect) value of one or fitting the data iteratively and updating the weights using the value of R_1 estimated at the previous iteration. We hypothesized that using the estimated R_1 would more accurately apportion the respective contributions of the target and reference region data to the total uncertainty of the residuals and thereby provide better results, but were initially surprised to find that the performance of Reference with R_1 iterated was intermediate between Standard and Reference weighting with R_1 fixed. This result can be explained by the severe underestimation of R_1 at high noise levels (figure 5). Note that the Reference weights given by equation (10) tend toward the Standard weights given by equation (9) as R_1 decreases, consistent with the intermediate performance of the Reference method when weighting factors were selected using the estimated value of R_1 (figure 4). Parameter bounds or constraints may improve the stability of the method in the presence of noise, but in the current formulation we recommend fixing R_1 when calculating Reference weighting factors.

5.2. Choice of the noise model

In this work, we have assumed that the uncertainty of the PET image data can be represented by Poisson-like distributions. Although Poisson statistics are strictly valid only at the event level, this approximation is employed frequently to model noise in the image domain for PET data analysis (e.g. Landaw and DiStefano 1984, Mazoyer *et al* 1986, Jovkar *et al* 1989, Delforge *et al* 1990, Chen *et al* 1991, Feng *et al* 1991, Vera *et al* 1992, Millet *et al* 1996). Alternative error approximations derived by empirical (Budinger *et al* 1978, Watabe *et al* 2000, Buvat 2002) and analytical (Alpert *et al* 1982, Huesman 1984, Defrise *et al* 1990, Carson *et al* 1993, Pajevic *et al* 1998, Qi 2003) procedures have been proposed and the development of more accurate models continues to be an active area of research. The most appropriate noise model is generally considered to be dependent on the acquisition type (2D versus 3D), reconstruction algorithm (e.g., filtered backprojection versus expectation maximization) and other physical factors such as voxel size, system resolution and detector design. It is not our intent in this paper to endorse the merits or generality of any particular noise model, and we note that the framework for Reference weighting described in this manuscript is generic and can be readily modified to accommodate whatever noise model is deemed most appropriate for the data at hand.

In implementing the Poisson noise model, we have calculated the variance based on the noisy data. This approach assumes that the PET measurement is a reasonable approximation of the true radioactivity concentration. This estimate is asymptotically correct for low noise levels, but its validity diminishes as noise increases. For this reason, it would be preferable to use iteratively reweighted least-squares or another technique that derives the weighting factors from the model fit rather than the measured data, particularly with noisier data (Spilker and Vicini 2001, Muzic and Christian 2006). Such approaches cannot be applied directly to the Reference weighting method because the SRTM provides a model fit to the target region data, but not to the reference region input function. Methods to obtain fits to both regions simultaneously are under investigation.

5.3. Assumptions and simplifications

We have made several assumptions that simplify the Reference method and improve its practical utility. The secondary terms in the BFM and MRTM operational equations were assumed to be effectively noiseless because integration effectively smooths noisy data (Ichise *et al* 2002). The noise in the target and reference region data was assumed to be uncorrelated. This approximation relies on the regions being sufficiently separated in space and the data being free of systemic error from reconstruction or motion artifacts. Finally, the error approximations were obtained from reconstructed image data only, in contrast with the method of Huesman and Mazoyer (1987), which was applied at the sinogram level to determine the variance of the PET data (Huesman 1984). While this approach is effective and elegant, the need to operate on sinograms, and in particular, to define ROIs in sinogram space, renders the method cumbersome in practice (Carson *et al* 1993). We believe that approximating the noise from the image data represents a reasonable tradeoff between accuracy and ease of use. As with the choice of noise model, the Reference weighting approach can be easily adapted if any of these simplifications are found to be invalid: the expression for the variance of the residuals could account for correlated noise or uncertain secondary terms in the operational equation by including the covariance or integral terms, and image-derived error approximations could be replaced with formulas that make use of sinogram data or other noise models, as described above.

6. Conclusions

The Reference weighting approach accounts for the statistical uncertainty of the reference region input function during selection of weighting factors. Simulation studies verified that Reference weighting improves SRTM performance at higher noise levels and when the target and reference regions are of comparable size. The region-based analysis of [¹¹C]flumazenil data from humans showed a small but significant increase in binding potential estimates when Reference weights were used and that the magnitude of the effect is associated with the relative sizes of the target and reference regions, consistent with the results of our simulation study. We have also shown with simulations that quantification of BP_{ND} may be improved by using a smaller, more appropriate reference tissue in tandem with Reference weighting. These results suggest that Reference weighting may be useful for small animal imaging, when injected radioactivity is limited by mass dose of tracer, or when a smaller reference tissue could be selected to avoid bias introduced by specific binding or partial volume effects. These benefits of Reference weighting may also apply to other models derived from the SRTM or to reference region methods, generally.

Acknowledgments

The authors acknowledge the support of the Society of Nuclear Medicine Student Fellowship Award to M D Normandin and NIH grant R21 AA015077 to E D Morris.

Appendix A. Derivation of Reference weighting

Assuming Poisson-like statistics, the variance of PET image data in a ROI can be approximated by equation (9). Hence the variances of the target and reference region radioactivity data at the i th frame of the dynamic PET series are given by

$$\sigma_{i,T}^2 = \zeta_T^2 \frac{C_T(t_i)}{n_T \Delta t_i} \quad (\text{A.1})$$

and

$$\sigma_{i,R}^2 = \zeta_R^2 \frac{C_R(t_i)}{n_R \Delta t_i}, \quad (\text{A.2})$$

where C is the measured tracer concentration and the subscripts T and R refer to the target and reference regions.

The residuals, r_i , are defined as the difference between the measured target region data, d_i , and the model predicted values, m_i :

$$r_i = d_i - m_i. \quad (\text{A.3})$$

A general expression for the variance of the residuals is given by

$$\text{var}\{r_i\} = \text{var}\{d_i\} + \text{var}\{m_i\} + 2 \cdot \text{cov}\{d_i, m_i\}. \quad (\text{A.4})$$

For our purposes, d_i corresponds to the measured target region PET data, $C_T(t_i)$, and m_i is given by the output of the BFM or MRTM operational equations shown in equations (7) and (8), respectively. Note that the basis functions of equation (7) contain a convolution term and equation (8) has two running integrals. Convolution smooths the data and integration sums them, both of which act as noise-reducing operators. We therefore regard the convolution and integral terms as effectively noiseless, and so equation (A.4) can be simplified to

$$\text{var}\{r_i\} = \text{var}\{C_T(t_i)\} + \text{var}\{R_1 C_R(t_i)\} + 2 \cdot \text{cov}\{C_T(t_i), R_1 C_R(t_i)\}. \quad (\text{A.5})$$

If we further assume that the statistical uncertainties of the target and reference region data are uncorrelated, the covariance term vanishes and the expression simplifies to

$$\begin{aligned} \text{var}\{r_i\} &= \text{var}\{C_T(t_i)\} + \text{var}\{R_1 C_R(t_i)\} \\ &= \text{var}\{C_T(t_i)\} + R_1^2 \text{var}\{C_R(t_i)\}. \end{aligned} \quad (\text{A.6})$$

Substituting equations (A.1) and (A.2) into equation (A.6) yields the expression for the variance of each residual as

$$\sigma_{i,\text{resid}}^2 = \zeta_T^2 \frac{C_T(t_i)}{n_T \Delta t_i} + R_1^2 \zeta_R^2 \frac{C_R(t_i)}{n_R \Delta t_i}. \quad (\text{A.7})$$

If the scaling factor ζ is constant (specifically, the same in the target and reference regions), we can let $\zeta_T = \zeta_R = \zeta$ and equation (A.7) simplifies to

$$\sigma_{i,\text{resid}}^2 = \frac{\zeta^2}{\Delta t_i} \left[\frac{C_T(t_i)}{n_T} + R_1^2 \frac{C_R(t_i)}{n_R} \right] \quad (\text{A.8})$$

which is identical to equation (10), the expression used to calculate the Reference weighting factors.

Appendix B. Example time activity curves for different noise levels

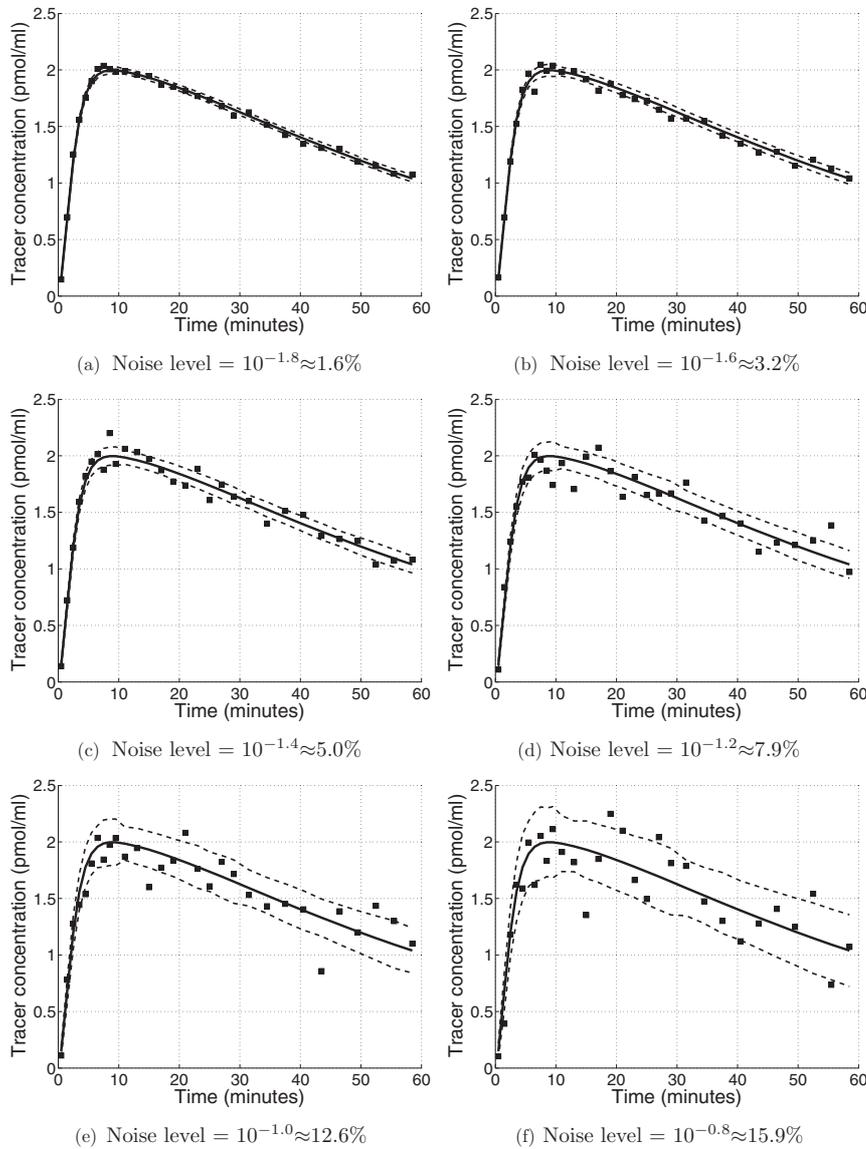


Figure B1. Simulated time activity curves over a range of noise levels. Markers depict a representative noisy time activity curve. Solid curve shows the noiseless time activity curve. Dashed curves form an envelope of one standard deviation about the mean at each time point across 500 noise replicates.

Appendix C. Alternative plots of performance as a function of noise level

Figures plotting bias \pm s.d. as a function of noise level at selected regions are shown as an alternative way to view a subset of the results presented in figures 2 and 3.

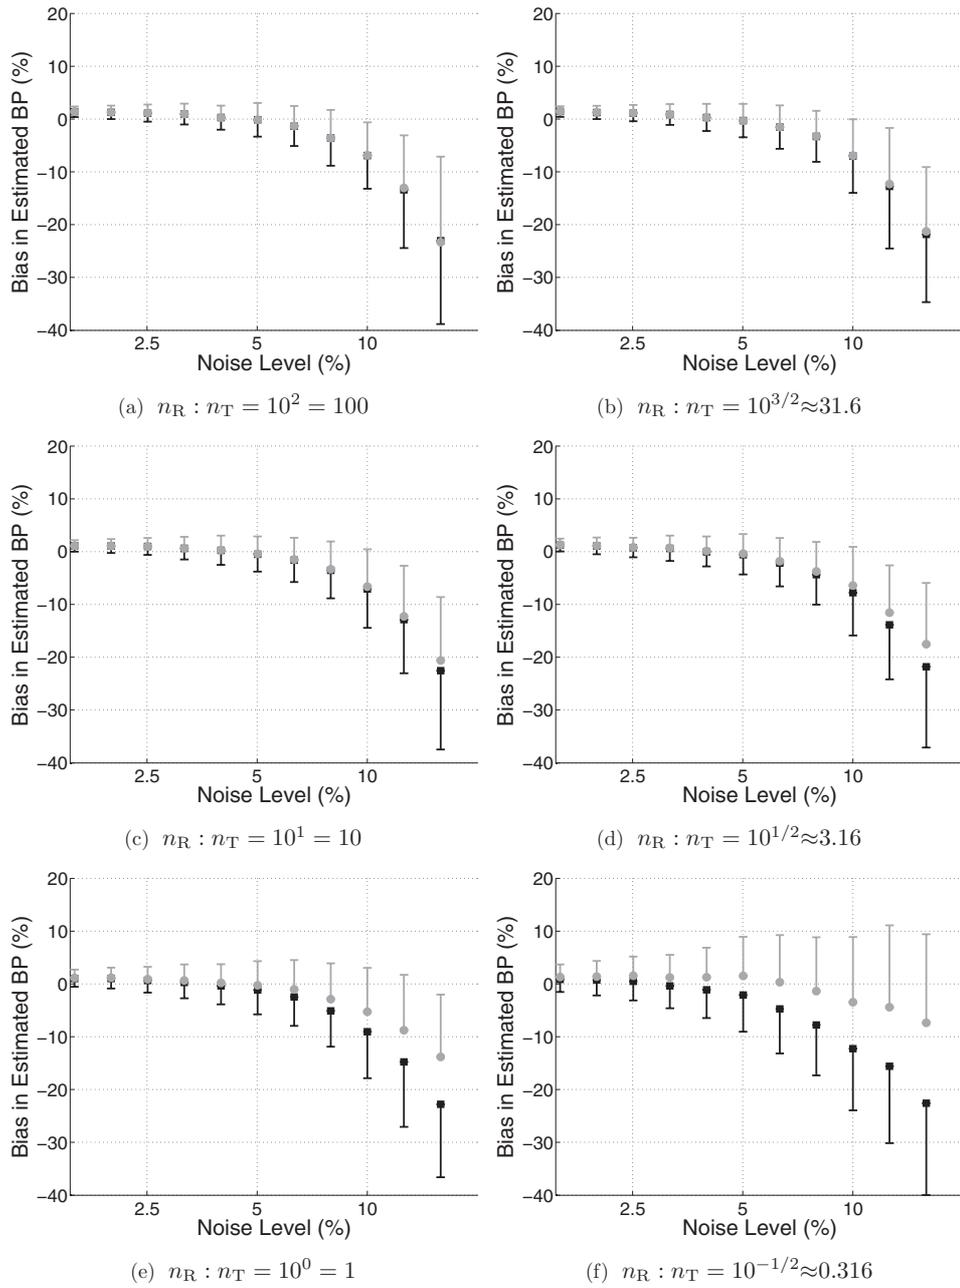


Figure C1. Bias of BP_{ND} as a function of noise level for estimates obtained using BFM with Reference (gray markers) or Standard weighting (black markers). Error bars represent the standard deviation across simulated data sets. The subplots each correspond to a different reference-to-target region volume ratio and collectively depict an alternative way to visualize a subset of the results presented in figure 2.

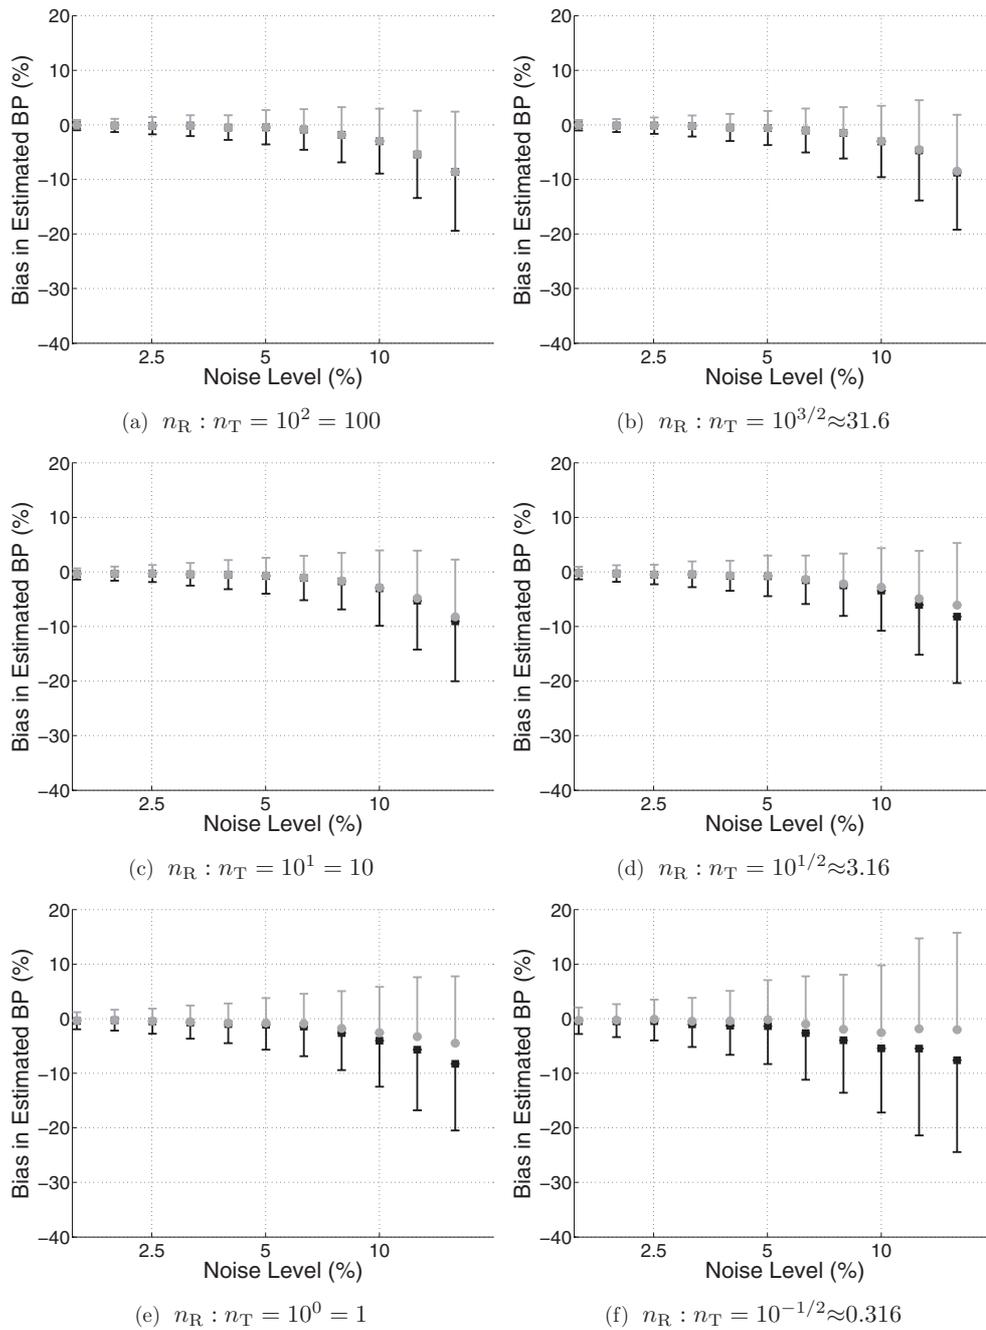


Figure C2. Bias of BP_{ND} as a function of noise level for estimates obtained using MRTM with Reference (gray markers) or Standard weighting (black markers). Error bars represent the standard deviation across simulated data sets. The subplots each correspond to a different reference-to-target region volume ratio and collectively depict an alternative way to visualize a subset of the results presented in figure 3.

References

- Alpert N M, Badgaiyan R D, Livni E and Fischman A J 2003 A novel method for noninvasive detection of neuromodulatory changes in specific neurotransmitter systems *Neuroimage* **19** 1049–60
- Alpert N M, Chesler D A, Correia J A, Ackerman R H, Chang J Y, Finklestein S, Davis S M, Brownell G L and Taveras J M 1982 Estimation of the local statistical noise in emission computed tomography *IEEE Trans. Med. Imaging* **1** 142–6
- Aston J A, Gunn R N, Worsley K J, Ma Y, Evans A C and Dagher A 2000 A statistical method for the analysis of positron emission tomography neuroreceptor ligand data *Neuroimage* **12** 245–56
- Blomqvist G, Pauli S, Farde L, Eriksson L, Persson A and Halldin C 1990 Maps of receptor binding parameters in the human brain—a kinetic analysis of PET measurements *Eur. J. Nucl. Med.* **16** 257–65
- Budinger T F, Derenzo S E, Greenberg W L, Gullberg G T and Huesman R H 1978 Quantitative potentials of dynamic emission computed tomography *J. Nucl. Med.* **19** 309–15
- Buvat I 2002 A non-parametric bootstrap approach for analysing the statistical properties of SPECT and PET images *Phys. Med. Biol.* **47** 1761–75
- Carson R E, Yan Y, Daube-Witherspoon M E, Freedman N, Bacharach S L and Herscovitch P 1993 An approximation formula for the variance of PET region-of-interest values *IEEE Trans. Med. Imaging* **12** 240–50
- Chen K W, Huang S C and Yu D C 1991 The effects of measurement errors in the plasma radioactivity curve on parameter estimation in positron emission tomography *Phys. Med. Biol.* **36** 1183–200
- Chiao P C, Rogers W L, Clinthorne N H, Fessler J A and Hero A 1994 Model-based estimation for dynamic cardiac studies using ECT *IEEE Trans. Med. Imaging* **13** 217–26
- Cunningham V J, Hume S P, Price G R, Ahier R G, Cremer J E and Jones A K 1991 Compartmental analysis of diprenorphine binding to opiate receptors in the rat *in vivo* and its comparison with equilibrium data *in vitro* *J. Cereb. Blood Flow Metab.* **11** 1–9
- Defrise M, Townsend D and Deconinck F 1990 Statistical noise in three-dimensional positron tomography *Phys. Med. Biol.* **35** 131–8
- Delforge J, Syrota A and Mazoyer B M 1990 Identifiability analysis and parameter identification of an *in vivo* ligand–receptor model from PET data *IEEE Trans. Biomed. Eng.* **37** 653–61
- Eaton J W 2002 *GNU Octave Manual* Network Theory Limited
- Feng D, Wang X, Fulton R, Hutton B and Morris J 1991 Effects of tracer blood measurement noise on glucose metabolic rate estimation *Biomed. Sci. Instrum.* **27** 43–8
- Gunn R N, Lammertsma A A, Hume S P and Cunningham V J 1997 Parametric imaging of ligand–receptor binding in PET using a simplified reference region model *Neuroimage* **6** 279–87
- Huesman R H 1984 A new fast algorithm for the evaluation of ROIs and statistical uncertainty in computed tomography *Phys. Med. Biol.* **29** 543–52
- Huesman R H 1997 Equivalent methods to analyse dynamic experiments in which the input function is noisy *Phys. Med. Biol.* **42** 147–53
- Huesman R H and Mazoyer B M 1987 Kinetic data analysis with a noisy input function *Phys. Med. Biol.* **32** 1569–79
- Ichise M, Cohen R M and Carson R E 2008 Noninvasive estimation of normalized distribution volume: application to the muscarinic-2 ligand [(18)F]FP-TZTP *J. Cereb. Blood Flow Metab.* **28** 420–30
- Ichise M, Liow J S, Lu J Q, Takano A, Model K, Toyama H, Suhara T, Suzuki K, Innis R B and Carson R E 2003 Linearized reference tissue parametric imaging methods: application to [11C]DASB positron emission tomography studies of the serotonin transporter in human brain *J. Cereb. Blood Flow Metab.* **23** 1096–112
- Ichise M, Toyama H, Innis R B and Carson R E 2002 Strategies to improve neuroreceptor parameter estimation by linear regression analysis *J. Cereb. Blood Flow Metab.* **22** 1271–81
- Ikoma Y, Watabe H, Hayashi T, Miyake Y, Teramoto N, Minato K and Iida H 2009 Quantitative evaluation of changes in binding potential with a simplified reference tissue model and multiple injections of [11C]raclopride *Neuroimage* **47** 1639–48
- Innis R B *et al* 2007 Consensus nomenclature for *in vivo* imaging of reversibly binding radioligands *J. Cereb. Blood Flow Metab.* **27** 1533–9
- Jovkar S, Evans A C, Diksic M, Nakai H and Yamamoto Y L 1989 Minimisation of parameter estimation errors in dynamic PET: choice of scanning schedules *Phys. Med. Biol.* **34** 895–908
- Koeppel R A, Holthoff V A, Frey K A, Kilbourn M R and Kuhl D E 1991 Compartmental analysis of [11C]flumazenil kinetics for the estimation of ligand transport rate and receptor distribution using positron emission tomography *J. Cereb. Blood Flow Metab.* **11** 735–44
- Lammertsma A A and Hume S P 1996 Simplified reference tissue model for PET receptor studies *Neuroimage* **4** 153–8

- Landaw E M and DiStefano J J III 1984 Multiexponential, multicompartmental, and noncompartmental modeling: II. Data analysis and statistical considerations *Am. J. Physiol.* **246** R665–77
- Mazoyer B M, Huesman R H, Budinger T F and Knittel B L 1986 Dynamic PET data analysis *J. Comput. Assist. Tomogr.* **10** 645–53
- Millet P, Delforge J, Pappata S, Syrota A and Cinotti L 1996 Error analysis on parameter estimates in the ligand–receptor model: application to parameter imaging using PET data *Phys. Med. Biol.* **41** 2739–56
- Minoshima S, Koeppe R A, Frey K A and Kuhl D E 1994 Anatomic standardization: linear scaling and nonlinear warping of functional brain images *J. Nucl. Med.* **35** 1528–37
- Minoshima S, Koeppe R A, Mintun M A, Berger K L, Taylor S F, Frey K A and Kuhl D E 1993 Automated detection of the intercommissural line for stereotactic localization of functional brain images *J. Nucl. Med.* **34** 322–9
- Mintun M A, Raichle M E, Kilbourn M R, Wooten G F and Welch M J 1984 A quantitative model for the *in vivo* assessment of drug binding sites with positron emission tomography *Ann. Neurol.* **15** 217–27
- Møller M, Rodell A and Gjedde A 2009 Parametric mapping of 5HT 1A receptor sites in the human brain with the hypotime method: theory and normal values *J. Nucl. Med.* **50** 1229–36
- Muzic R F Jr and Christian B T 2006 Evaluation of objective functions for estimation of kinetic parameters *Med. Phys.* **33** 342–53
- Normandin M D, Schiffer W K and Morris E D 2011 A linear model for estimation of neurotransmitter response profiles from dynamic pet data *Neuroimage* (at press)
- Pajevic S, Daube-Witherspoon M E, Bacharach S L and Carson R E 1998 Noise characteristics of 3D and 2D PET images *IEEE Trans. Med. Imaging* **17** 9–23
- Qi J 2003 A unified noise analysis for iterative image estimation *Phys. Med. Biol.* **48** 3505–19
- Snyder D L 1973 Statistical analysis of dynamic tracer data *IEEE Trans. Biomed. Eng.* **20** 11–20
- Spilker M E and Vicini P 2001 An evaluation of extended vs weighted least squares for parameter estimation in physiological modeling *J. Biomed. Inform.* **34** 348–64
- Thiele F and Buchert R 2008 Evaluation of non-uniform weighting in nonlinear regression for pharmacokinetic neuroreceptor modelling *Nucl. Med. Commun.* **29** 179–88
- Tomasi G, Bertoldo A, Schmidt K, Turkheimer F, Smith C and Cobelli C 2008a Residual-based comparison of different weighting schemes for pixel-wise kinetic analysis at the pixel level in PET *Neuroimage* **41** T84
- Tomasi G, Edison P, Bertoldo A, Roncaroli F, Singh P, Gerhard A, Cobelli C, Brooks D J and Turkheimer F 2008b Novel reference region model reveals increased microglial and reduced vascular binding of 11C-(R)-PK11195 in patients with Alzheimer’s disease *J. Nucl. Med.* **49** 1249–56
- Vera D R, Scheibe P O, Krohn K A, Trudeau W L and Stadelnik R C 1992 Goodness-of-fit and local identifiability of a receptor-binding radiopharmacokinetic system *IEEE Trans. Biomed. Eng.* **39** 356–67
- Watabe H, Endres C J, Breier A, Schmall B, Eckelman W C and Carson R E 2000 Measurement of dopamine release with continuous infusion of [¹¹C]raclopride: optimization and signal-to-noise considerations *J. Nucl. Med.* **41** 522–30
- Wu Y and Carson R E 2002 Noise reduction in the simplified reference tissue model for neuroreceptor functional imaging *J. Cereb. Blood Flow Metab.* **22** 1440–52
- Zhou Y, Chen M K, Endres C J, Ye W, Brasic J R, Alexander M, Crabb A H, Guilarte T R and Wong D F 2006 An extended simplified reference tissue model for the quantification of dynamic PET with amphetamine challenge *Neuroimage* **33** 550–63
- Zhou Y, Endres C J, Brasic J R, Huang S C and Wong D F 2003 Linear regression with spatial constraint to generate parametric images of ligand–receptor dynamic PET studies with a simplified reference tissue model *Neuroimage* **18** 975–89